



## Portable Data Logger with 30 Standard Channels Expandable to 60 Channels

Only the size of an A4 sheet of paper, the HIOKI LR8400-20 Series is the realization of our goal to build a logger that provides the existing functionality of a multi-channel data logger in a portable format. The new model comes with 30 channel capability as standard, to which another 30 channels can be added. All input channels for measuring temperature (with thermocouples), or voltage are isolated for safety, culminating in a powerful multi-measurement system that also offers pulse and logic inputs. Long-term logging is coupled with the capability to protect data against unexpected power outages and other problems for stable recordings over an entire year (see note).

*Note: Continuous recordings lasting longer than 1 year are also possible.*

# In fuel cell, electric automobile and other development

Provides assistance with

- Environmental measurements to prevent global warming
- Development of fuel cell materials, energy field
- Development of automobiles, testing of automobile parts
- Maintenance and inspection of equipment
- Monitoring plants
- Testing of electrical products
- Impedance testing of electronic parts

## Multi-channel measurements

In the development of fuel cells, multiple power-generating cells are connected to form a stack. Independent measurements of each cell require multi-channel measurements of DC voltage, DC current, temperature and other parameters. The LR8400-20 Series comes with 30 channels as standard, which can be expanded to 60 channels.

## High withstand voltage

The HiLOGGER measures not only fuel cells, but also batteries for UPS (uninterruptible power supplies) devices used in buildings as well as batteries consisting of cells and packaging connected in stacks that require multi-point measurements.


In such measurements, high voltage for the whole stack is applied between channel-to-channel and channel-to-ground. Only a measuring instrument with isolated inputs and high-capacity withstand voltage characteristics can endure this.

Note: Isolation between channels is possible through the use of semi-conductor relays. Voltage exceeding the product specifications, such as that originating from lightning surges or other sources, should never be applied between each channel; otherwise the relays will short and the recorder will be damaged.

## High-speed sampling

In the development of automobiles such as electric vehicles (EV) and plug-in hybrid vehicles (PHV) that use motors for propulsion, abrupt changes in load need to be measured.

This makes the multi-channel, high-speed 10 ms sampling capability of the LR8400-20 Series an indispensable feature.

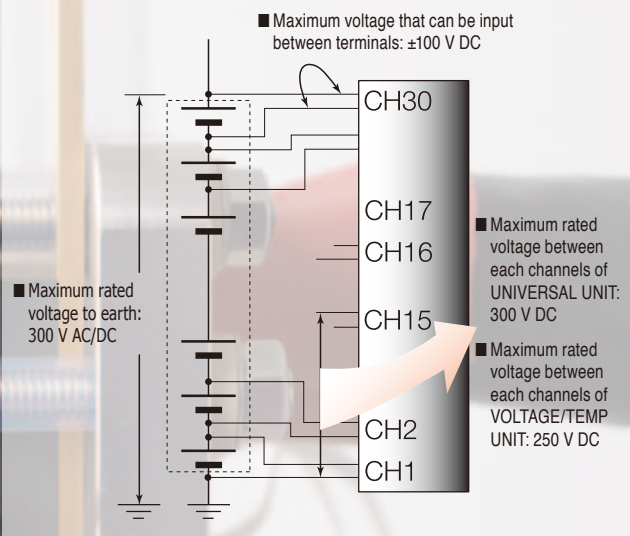

# Highlights

Multi-measurements

## Measure and record:

- Temperature & humidity
- A variety of transducer outputs (DC voltage)
- Resistance values

Also comes with high withstand voltage; isolated inputs required when measuring and recording battery cell voltages

### Voltage measurement (DC only)

- 30 input channels

Note: The LR8400-20, LR8401-20 and LR8402-20 models differ in the combination of input functions and terminals.

- All input channels are isolated

Note: Maximum rated voltage above ground between the HiLOGGER and analog inputs is 300 V AC/DC.

Note: Maximum channel-to-channel voltage is a high voltage of 300 V DC. (Maximum voltage for models with M3 screw input terminals is 250 V DC.)



### Temperature & humidity measurement

- Temperature measurements of thermocouples on 30 channels
- M3 screw terminal inputs enable secure connection of even thin thermocouples
- Special sensor permits humidity measurements on 30 channels (optional Z2000)

Note: The sensor power supply is the M3 mm dia. screw terminal block on the left side. Note: Both universal input terminals and M3 mm dia. input terminals enable humidity measurements.




### Temperature & resistance measurement


- Universal inputs support temperature measurements using Platinum resistance temperature sensor (Pt100/ JPt100), or resistance measurements (four wires)

Note: These cannot be measured using the M3 screw input terminals units.

Note: Supports resistance recording to enable assessment of changes in resistance in the device under test. 4-terminal method, measurement resolution 0.5 mΩ, testing current 1 mA



To record 4 - 20mA instrumentation signals, attach a commercially available 250Ω shunt resistance to the input terminals (between + and -) to convert the signals to 1 - 5V. Then use the 1-5V or the 10V f.s. input range in the HiLOGGER.



### ■ A compact A4 size enhances mobility

A compact A4 size footprint makes it ideal for use in virtually any environment.

### ■ Helps also in collecting automotive data

Ideal for testing and collecting data on the vibration characteristics of automotive parts



### Pulse totalization measurement

- 8 channel inputs (pulse and digital input selectable for each channel)
- For measuring energy consumption and cumulative flow

The input signal shares common ground with the HiLOGGER  
Note: M3 screw input terminals provide direct connection



### Pulse rotations measurement

- 8 channel inputs (pulse and digital input selectable for each channel)
- For measuring rotational irregularities of motors and drills


The input signal shares common ground with the HiLOGGER  
Note: M3 screw input terminals provide simple connection



### Logical 1-0 measurement

- 8 channel inputs (digital and pulse input selectable for each channel)
- 1 or 0 is recorded for each recording interval

The input signal shares common ground with the HiLOGGER  
Note: M3 screw input terminals provide simple connection






# Accurately capture any phenomena you want to measure

## Highlights

### High-speed Recording

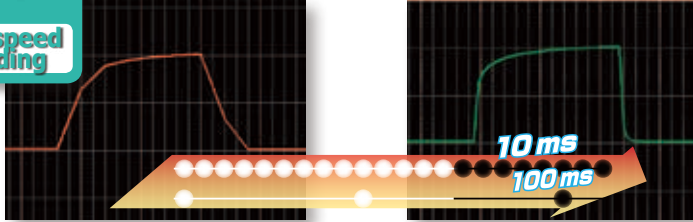

Sampling at 100 ms intervals cannot capture abrupt load changes

Sampling the same waveform at ten times the speed, at 10 ms intervals, accurately captures the changes.


### ■ 10 ms high-speed sampling

The development of hybrid and electric automobiles requires instruments that can measure abrupt load changes. Channels 1 to 15 provide 10-ms sampling and channels 16 to 30 provide 20-ms sampling. These channels allow you to track waveforms not possible with earlier models.

*Note: Measurements on channels 31 to 60 provide 50-ms sampling.*

## Highlights

### Noise suppression

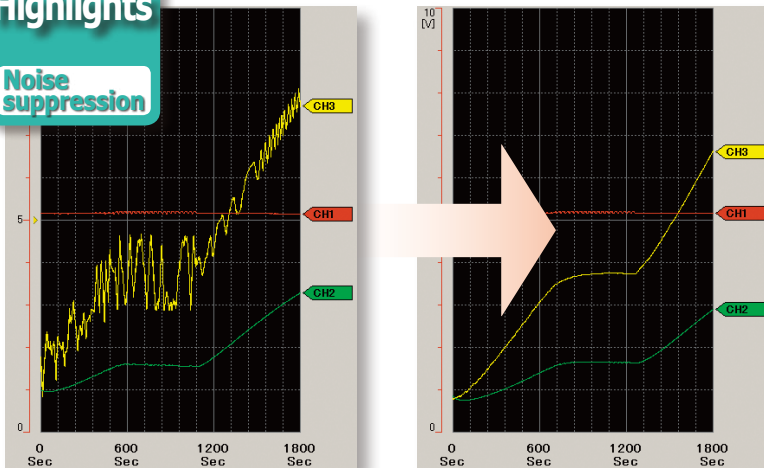

Without electric noise reduction, you will obtain a waveform like the one above in temperature measurements of an electromagnetic cooker

A digital filter in the HiLOGGER eliminates high-frequency noise to enable accurate temperature waveforms

### ■ Enhanced noise suppression

A digital oversampling filter function reduces inverter switching noise and 50/60 Hz hum noise, a concern in earlier models, during recording.

*Note: The noise reduction effect improves with longer recording intervals (i.e., at slower sampling speeds).*

## Highlights


### Easy-to-view LCD



### ■ 5.7 inch TFT LCD display is easy to view even at an angle

The LCD has a wider visual angle and is larger (5.7 inches, 640 × 480 dots)

than the STN LCD in our previous model (8420-51s) to facilitate observation of waveforms on multiple channels.

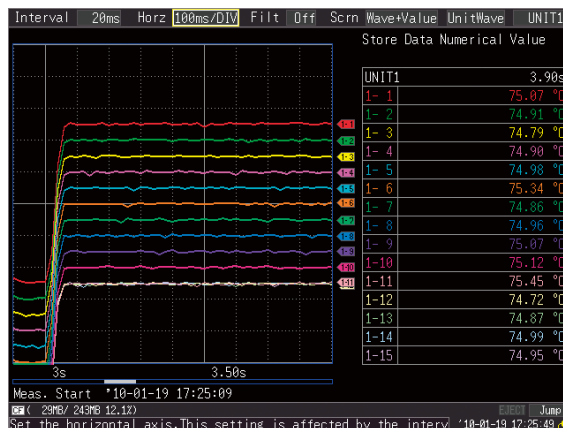

# Store data securely for more than 1 year

## Highlights

### Storage Media



### Compatible with USB memory devices

For even greater convenience, the HiLOGGER now provides support for USB memory devices. Measurements can now immediately be written to a USB memory device in real-time. USB memory devices are also a handy means to transfer data to a PC.

*Note: Although USB memory devices enable real-time saving of data, for more reliable data protection we recommend use of HIOKI CF cards, which are guaranteed to work with the instrument, for real-time saving of data.*

### Saving data to CompactFlash (CF) card

Use only HIOKI CF cards, which are manufactured to strict industrial standards, for long-term storage of important data.

*Note: Operation of non-HIOKI CF cards is not guaranteed*



### Recording Capacity

*Note: Use only HIOKI CF cards that are guaranteed to operate with the HiLOGGER for continuous long-term recording.*

| Recording intervals                          | Recording of 15 analog channels only (no pulse measurement, alarm output or waveform processing data) |                     |                   |                   |
|--|---|---------------------|-------------------|-------------------|
|  | Internal memory (16 MB)   | Model 9728 (512 MB) | Model 9729 (1 GB) | Model 9830 (2 GB) |
| 10 ms *<br>* For 15 or fewer analog channels | 1h 33m  | 2d 01h 42m          | 4d 03h 25m        | 8d 06h 50m        |
| Recording intervals                          | Recording of 30 analog channels only (no pulse measurement, alarm output or waveform processing data) |                     |                   |                   |
|  | Internal memory (16 MB)   | Model 9728 (512 MB) | Model 9729 (1 GB) | Model 9830 (2 GB) |
| 20 ms *<br>* For 30 or fewer analog channels | 1h 33m  | 2d 01h 42m          | 4d 03h 25m        | 8d 06h 50m        |
| 50ms   | 3h 53m  | 5d 04h 16m          | 10d 08h 33m       | 20d 17h 06m       |
| 100ms  | 7h 46m  | 10d 08h 33m         | 20d 17h 06m       | 41d 10h 12m       |
| 200ms  | 15h 32m   | 20d 17h 06m         | 41d 10h 12m       | 82d 20h 24m       |
| 500ms  | 1d 14h 50m  | 51d 18h 45m         | 103d 13h 30m      | 207d 03h 01m      |
| 1s   | 3d 05h 40m  | 103d 13h 30m        | 207d 03h 01m      | 414d 06h 03m      |
| 2s   | 6d 11h 20m  | 207d 03h 01m        | 414d 06h 03m      | "★"               |
| 5s   | 16d 04h 21m   | 517d 19h 34m        | "★"               | "★"               |
| 10s  | 32d 08h 43m   | "★"                 | "★"               | "★"               |
| 20s  | 64d 17h 26m   | "★"                 | "★"               | "★"               |
| 30s  | 97d 02h 10m   | "★"                 | "★"               | "★"               |
| 1min   | 194d 04h 20m  | "★"                 | "★"               | "★"               |
| 2min   | 388d 08h 40m  | "★"                 | "★"               | "★"               |
| 5min to 1hour                                | "★"   | "★"                 | "★"               | "★"               |

- Maximum recording time is inversely proportional to number of recording channels.
- Because the actual capacity of a CF card is less than that indicated, and because the header portion of waveform files is not included in capacity calculations, expect actual maximum times to be about 90% of those in the table.
- "★" exceeds 1 year.

## Highlights

### Replacing cards



### Cards can be replaced during real-time recording

This function has been provided to enable removal of cards during recording to allow the user to analyze the data recorded so far. This makes it possible to replace USB memory devices and CF cards during real-time recording without having to stop measurements.

*Note: During high-speed recording, be sure to insert the new storage media within 2 minutes of removing a card.*

# A host of useful functions and features



- VOLTAGE/TEMP UNIT LR8500**
- 15ch
  - M3 screw terminals (2 terminals per channel)
- UNIVERSAL UNIT LR8501**
- 15ch
  - Push-button type terminals (4 terminals per channel)



## ■ Up to two additional 15 channel input units can be added

The need for more measurement channels can be met even after purchasing the instrument. The instrument comes with 30 channels as standard, but another two 15 channel input units can be added to expand the total number of channels to 60.


*Note: The units provided with the unit as standard cannot be removed.*

The number of input channels  
can be expanded!!  
**Max. 60 ch**



## Function highlights


**Ease of use**

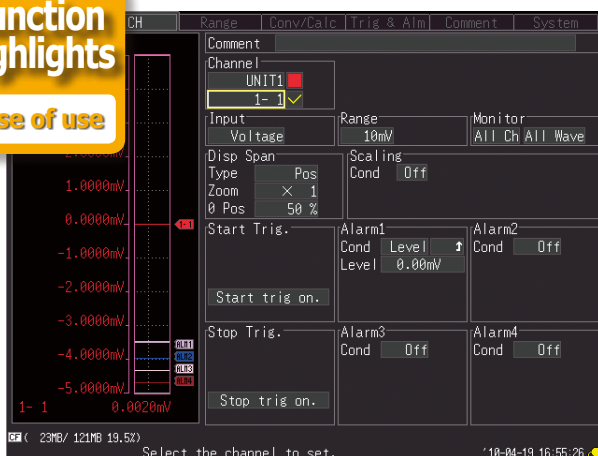

## ■ Input setting screens with waveform monitoring

The HiLOGGER adopts the setting screens that earned its sister model (8430-20) a reputation for user-friendliness. Range settings, warnings, triggers, waveform processing and other measurement input settings can be taken in at a glance.




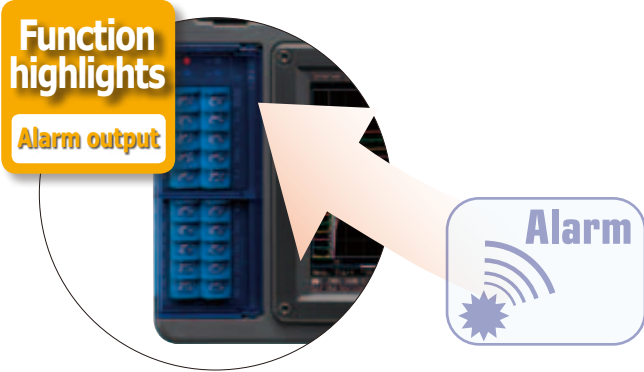

■ Alarm output

The HiLOGGER outputs a signal when alarm criteria are satisfied and also sounds a buzzer. Four systems are provided as standard and separate criteria can be set for each input source enabling OR and AND criteria between channels.

*Note: Open-collector output (5 V voltage output and relay drive capacity 5 to 30 V, 200 mA)*

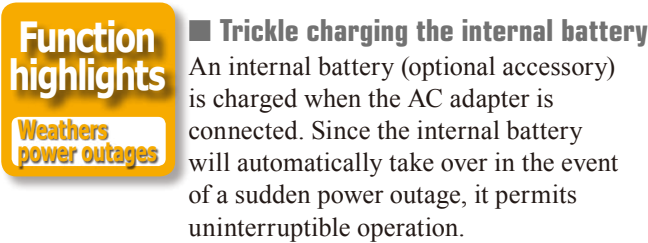


■ Trickle charging the internal battery

An internal battery (optional accessory) is charged when the AC adapter is connected. Since the internal battery will automatically take over in the event of a sudden power outage, it permits uninterrupted operation.

■ Protection of files being stored on external storage media

An internal high-capacity capacitor will provide enough power to store any data at risk on a CF card or USB memory device should a sudden power outage occur during long-term storage. This reduces the risk of data loss and corruption of the file system. Measurements will resume as soon as the power returns.

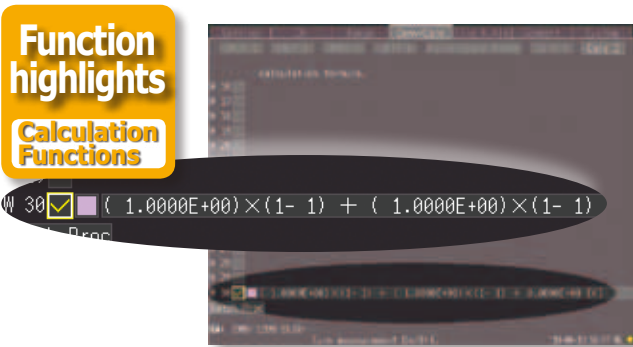


■ Real-time processing functions

The HiLOGGER comes with [four arithmetic operation] functions for processing between channels. Data processed in real-time can be displayed in graph form. In addition, processing results for 30 channels are stored in internal memory and can be handled as data for independent input channels.

■ Records average values every 30 minutes

The HiLOGGER contains a [time-span processing] function. The instrument will save processing data as text data for a preset time period in real-time.

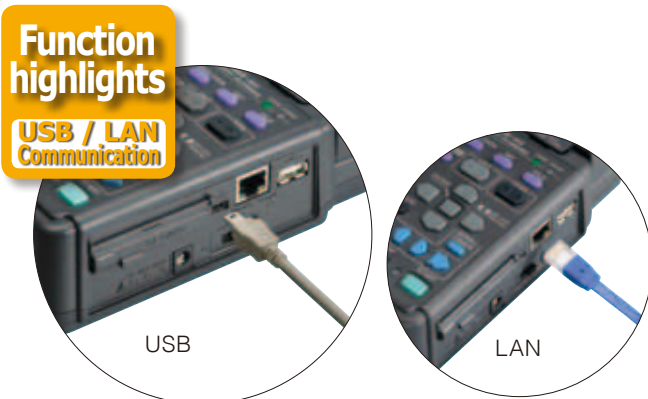

■ Simultaneous recording to storage media and PC

Measurement data can be simultaneously saved to external storage media and a hard disk on a PC connected to a network to reduce the risk data loss.




■ USB and LAN connection for easy setup

The supplied Logger Utility software allows you to set up the logger from a PC. Setup could not be easier. Just follow the numbered procedures to set up the instrument.

*Note: Data on an inserted CF card can be copied to a PC via USB connection.*


*Note: The Logger Utility will enable LAN access with software Ver. 1.20 or later.*

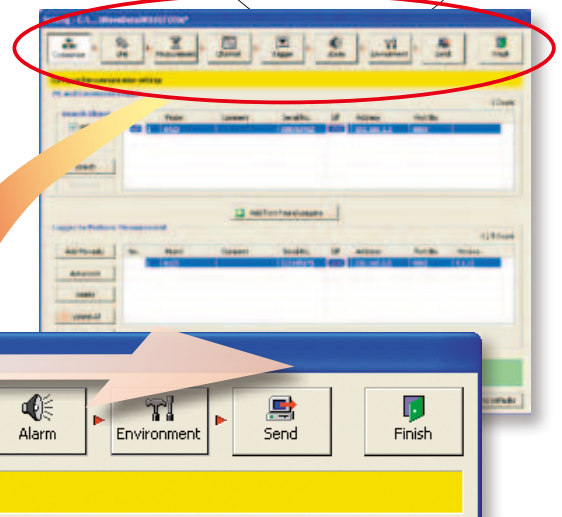

# Bundled user-friendly software for PC analysis


**Function highlights**  
PC Measurement

- The supplied Logger Utility software enables processing of measurement data on a PC
- View past data during recording
- Output PC data to a printer

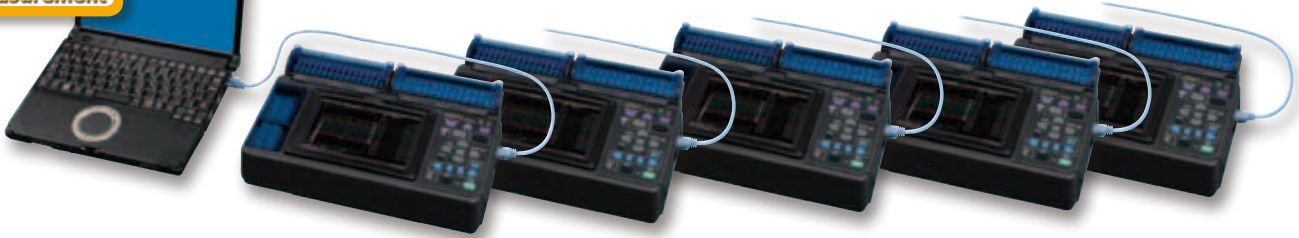


## ■ Control of measurements from a PC screen

Connect the PC to the HiLOGGER using USB or via LAN\* (see note). Use the supplied Logger Utility software to record data on a PC in real-time. Scroll backwards through the displayed trend graph window to view past waveforms even while recording. Up to five HiLOGGERS can be connected to one PC.

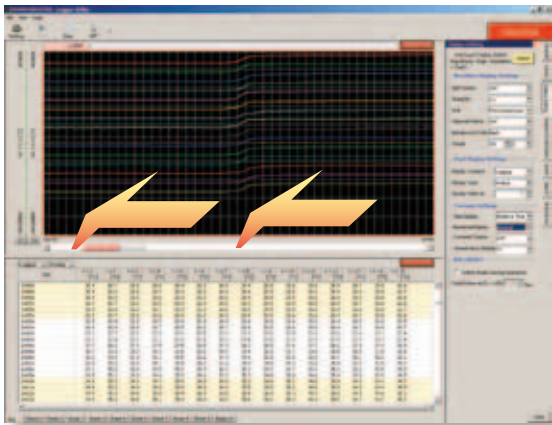

## ■ Analyze after measuring

Our new “dual-knob function” greatly simplifies data analysis. Two separate waveform windows are provided, with the displayed waveforms showing different time-axis scales (time bases). This capability substantially simplifies long-term data analysis.

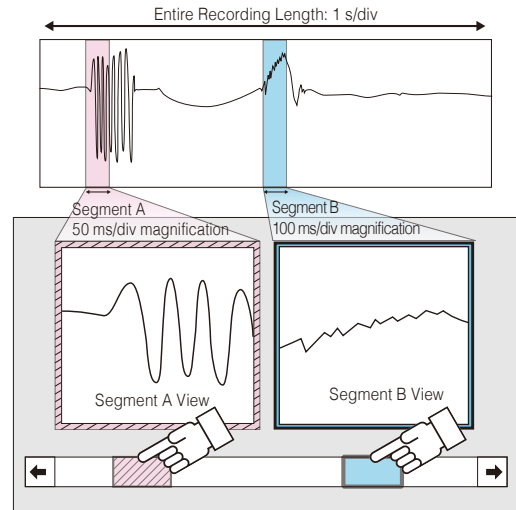

## ■ Remote control through HTTP server function\*


Without the need to install additional software, you can use an ordinary web browser on your PC to set up the HiLOGGER, acquire data and monitor data on the screen.

*Note: Waveform data cannot be downloaded from internal memory while measuring.*

## ■ Data acquisition via FTP\*

FTP allows the PC to acquire files stored on HiLOGGER storage devices or measurement data in internal memory.

*Note: Waveform data cannot be downloaded from internal memory while measuring.*

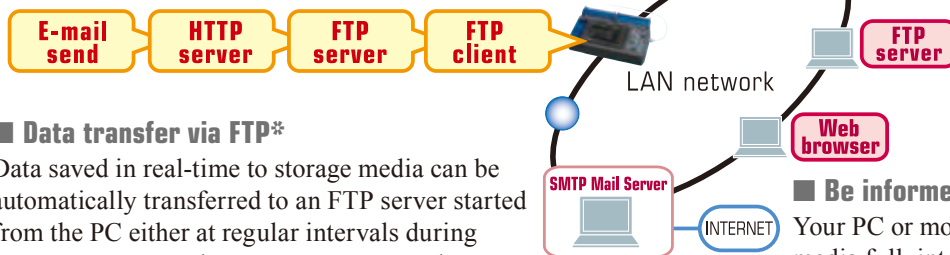

## ■ Data transfer via FTP\*

Data saved in real-time to storage media can be automatically transferred to an FTP server started from the PC either at regular intervals during measurements or when measurements end.

## ■ Be informed via E-mail\*

Your PC or mobile device is notified of storage media full, internal memory full, stop trigger invoked, alarm occurrence and other events via E-mail.

\*Note: LAN communication functions support planned from software Ver. 1.20.



## Product Specifications


| General specifications   |   |
|--|---|
| (product and accuracy guaranteed for 1 year, post-adjustment accuracy guaranteed for 1 year) |   |
| Internal memory  | 16 Mega-bytes (8M data points)  |
| Internal clock   | Auto calendar, Precision $\pm 3$ s/ day (at 23 °C/ 73 °F)   |
| Accuracy of timebase   | $\pm 0.2$ s/ day on measurement (at 23 °C/ 73 °F)   |
| Backup battery   | For clock and setting conditions: battery life 5 years (at 23 °C/ 73 °F)  |
| Operating temp. & humidity   | 0 °C (32 °F) to 40 °C (104 °F), 80% rh or less (non-condensating, when charging: 10 °C/ 50 °F to 40 °C/ 104 °F)   |
| Storage temp. & humidity   | -10 °C (14 °F) to 60 °C (140 °F), 80% rh or less, (non-condensating)  |
| Conforming standards   | Safety : EN61010, EMC : EN61326, EN61000-3-2, EN61000-3-3   |
| Anti-vibration   | JIS D1601: 1995 5.3 (I) Corresponds to Class 1: a passenger car, Condition: class A   |
| External control terminal  | External trigger input, Trigger output, 4 channel alarm outputs, +12 V/ 100 mA max. output, GND   |
| Dimensions & Mass  | Approx. 272 mm (10.71 in) W $\times$ 182.4 mm (7.18 in) H $\times$ 66.5 mm (2.62 in) D, 1.8 kg (63.5 oz), (LR8400 main unit, except the Battery Pack 370 g/ 13.1 oz)<br>Approx. 272 mm (10.71 in) W $\times$ 234.8 mm (9.24 in) H $\times$ 66.5 mm (2.62 in) D, 2.6 kg (91.7 oz), (LR8500 $\times$ 2 and LR8400 $\times$ 1, except the Battery Pack 370 g/ 13.1 oz)   |
| Accessories  | Detailed operating manual $\times$ 1, Measurement guide $\times$ 1, AC ADAPTER 9418-15 $\times$ 1, USB cable $\times$ 1, CD-R (data collection software "Logger Utility") $\times$ 1  |
| Data storage media   |   |
| CF card  | CF card slot $\times$ 1 (Up to 2GB), Data format: FAT, FAT32  |
| USB memory   | Series A receptacle   |
| Communication function   |   |
| LAN interface<br>(ver. 1.20 or later)  | IEEE 802.3 Ethernet 100BASE-TX, DHCP, DNS capable<br>• Data acquisition, condition settings used with the Logger Utility software (supplied as standard)<br>• Use the communication command to set and measure<br>• Data download via FTP server function (stored in the CF card or the USB memory)<br>• Automatically transmit data via FTP client function<br>• Remote control via HTTP server function<br>• Send mail function via E-mail system |
| USB communication interface  | USB 2.0 High-speed capable, series mini-B receptacle<br>• Data acquisition, condition settings used with the Logger Utility software (supplied as standard)<br>• Configure the unit and measure using communication commands<br>• Transfer data from the CF card to a PC via USB drive mode (data transfer not possible from USB memory sticks)   |
| Display section  |   |
| Display device   | 5.7 inch TFT color liquid crystal display (640 $\times$ 480 pixel), horizontal 15 division, vertical 10 division, selectable between English and Japanese displays, Back light saver available  |
| LCD Brightness   | Selectable from 100, 70, 40, or 25%   |
| Power supplies   |   |
| AC Power   | Using the AC ADAPTER 9418-15 (supplied as standard, 100 to 240 VAC, 50/60 Hz),<br>Power consumption: 7 VA (with battery pack removed and maximum brightness)  |
| DC Power   | Using the BATTERY PACK Z1000 (optional accessory, 7.2 V, AC adapter has priority when used in combination with battery pack)<br>Continuous operation time: 5 hours (at 23 °C, LCD brightness 25%)<br>Fast recharging time: 3 hours (using the AC adapter and main unit to recharge the battery, at 23 °C, reference value)  |
| External   | 10 to 28 VDC (Rechargeable voltage 12 to 16 VDC, Please contact your HIOKI distributor for connection cord)<br>Maximum rated power: 24 VA (at 16 VDC external power supply, battery charge, LCD brightness 100%)  |
| Trigger functions  |   |
| Trigger mode, timing   | Modes : Single / Repeat, Timing : Start / Stop / Start & Stop, Logical sum (OR) and product (AND) of each trigger source, Selectable for each channel   |
| Analog signal source   | Configure each individual channel for 30 channels or up to 60 channels depending on number of additional terminal modules installed.<br>[Level trigger] Triggers when rising or falling through preset level<br>[Window] Triggers when entering or exiting range defined by preset upper and lower limit values   |
| Pulse signal source  | 8 channels of pulse totalizer inputs<br>[Level trigger] Triggers when rising or falling through preset level<br>[Window] Triggers when entering or exiting range defined by preset upper and lower limit values   |
| Digital signal source  | 8 channels of digital signal inputs<br>[Logic pattern trigger] agreement (or disagreement) in the specified [1/ 0/ $\times$ ] pattern   |
| Timer trigger  | Set up for year/ month/ day/ hour/ minute/ second   |
| Trigger output   | Open collector (active low, with 5 V output, at least 10 ms pulse width), M3 mm screw terminal  |
| Alarm output   |   |
| Number of channels   | 4 channels, non-isolated (common ground with chassis)   |
| Alarm source   | 60 channels of analog input, 8 channels of pulse totalizer inputs or digital inputs, Thermocouple burn-out detection  |
| Alarm type   | Level, Window, Logic pattern, Output latch/ no latch, Cancel alarm while measuring  |
| Alarm sound  | Buzzer, ON/OFF possible   |
| Alarm output   | Open collector (active low, with 5 V output), M3 mm screw terminal, Output refreshed at every recording interval  |
| Output sink current  | 200 mA at 5 V to 30 VDC   |

| Measurement Settings                  |   |                   |                       |
|---------------------------------------|---|-------------------|-----------------------|
| Recording Intervals (sampling period) | 10 ms <sup>*1</sup> , 20 ms <sup>*2</sup> , 50 ms <sup>*3</sup> , 100 ms to 1 hr (19 selections)<br>Note: All input channels are scanned within each recording interval<br><sup>*1</sup> Thermocouple burn-out detection OFF, and using up to 15 channels<br><sup>*2</sup> Thermocouple burn-out detection OFF, and using up to 30 channels, or Thermocouple burn-out detection ON, and using up to 15 channels<br><sup>*3</sup> Thermocouple burn-out detection OFF, and using up to 60 channels, or Thermocouple burn-out detection ON, and using up to 30 channels |                   |                       |
| Graph time axis                       | 100 ms/ div to 1 day/ div (21 selections)<br>Note: Setting is independent from the recording interval   |                   |                       |
| Recording Time                        | Enable continuous recording ON (records until the Stop key is pressed), or continuous recording OFF (enable a specified time span)  |                   |                       |
| Repeating Recording                   | (ON/OFF) Enable to repeat recording after the specified recording time span has elapsed   |                   |                       |
| Data Saving                           |   |                   |                       |
| Storage media                         | Select a CF card or USB memory (Use only PC Cards sold by HIOKI)  |                   |                       |
| Storage operation                     | Auto: Save waveform data or time divided calculation results in real time<br>Manual: Push the save key (operation select: item choose/ directly save)   |                   |                       |
| Real-time saving                      | Possible: Waveforms are saved approximately one minute as binary or text data to the CF card or the USB memory (if sampling rate is slower than 1 minute, waveforms are saved at each interval)<br>To the PC: Waveforms are saved to the HDD in the PC via LAN or USB communication when used with the Logger Utility Software. Data can be saved in real time to the CF card or USB memory at the same time.   |                   |                       |
| Divided saving                        | Simple divide: Save waveform data at pre-set times into separate files from the time measurement starts.<br>On schedule: Designate a reference time within 24 hours and save data into separate files at every set time interval starting from the reference time.  |                   |                       |
| Delete & save                         | Endless loop saving: New file overwrites the oldest file when the CF card or USB memory capacity runs short   |                   |                       |
| Interruptions during saving           | Storage media may be removed during real-time save after message confirmation.<br>Upon inserting the storage media again, data saved in internal memory during that time will be saved as a separate file in the media.   |                   |                       |
| Data protect                          | Possible: When a power failure occurs during real-time save, the file close sequence is completed before the unit is shut down. When powering with batteries and low battery power is detected, the file close sequence will automatically be executed.   |                   |                       |
| Saved data types                      | Setting condition, Waveform data (binary or text style), Calculation of numerical value, Screen data (compressed BMP)   |                   |                       |
| Loading data                          | Stored binary data can be recalled by the HiLOGGER in 16 MB quantities  |                   |                       |
| Calculation function                  |   |                   |                       |
| Numerical value calculations          | No. 1 to 6, maximum 6 calculations can be conducted simultaneously<br>Selections: average value, peak value, maximum value, time at maximum value, minimum value, time at minimum value   |                   |                       |
| Data range of calculation             | All data in internal memory: While measuring/ After measuring<br>Between A/B cursors: After measuring<br>Times: Calculate values at pre-determined 1 sec to 1 day intervals and display the latest value  |                   |                       |
| Calculation value save                | Possible: After measuring the last calculated value is automatically saved to the CF card or USB memory as a text file<br>Timed save: Save calculated data at pre-determined 1 sec to 1 day intervals as text data to the CF card or USB memory in real time.   |                   |                       |
| Waveform calculations                 | <sup>*4</sup> arithmetic calculations between each channel<br><sup>*5</sup> Separate display of calculation graphs (only during measurement) and input waveforms<br><sup>*6</sup> Real-time save of calculation graph data  |                   |                       |
| Other functions                       |   |                   |                       |
| Event marking                         | Search: Move to the event number entered and display the waveforms appearing before and after event<br>Number of events: Maximum 100 per measurement  |                   |                       |
| A-B cursor                            | Measurement: time difference between A and B, electric potential difference, electric potential of A or B and time<br>Type: Trace the data, amplitude axis, time axis   |                   |                       |
| Scaling                               | Convert and display the measurement value of each channel as a scaled value   |                   |                       |
| Rate adjustment                       | Scaling can be set for a channel so that its value is the same as that for UNITI-CHI  |                   |                       |
| Comment input                         | Enter a title or a comment for each channel   |                   |                       |
| Other                                 | Start backup, save ten types setting conditions into main unit, auto set up, start/stop key lock, key-lock, beep sound  |                   |                       |
| Pulse, Digital input                  |   |                   |                       |
| Number of channels                    | 8 channels, (digital / pulse selectable for each channel, M3 screw terminal $\times$ 8ch, 2 terminals per channel, not isolated, common ground)   |                   |                       |
| Input condition                       | No-voltage 'a' contact (normally open contact), open collector or voltage input, Input resistance: 1.1 M $\Omega$   |                   |                       |
| Max. allowable input                  | 0 V to 50 VDC (maximum voltage between input terminals that does not cause damage)  |                   |                       |
| Max. rated voltage between channels   | Not isolated (common ground)  |                   |                       |
| Max. rated voltage to earth           | Not isolated (common ground)  |                   |                       |
| Detect level                          | 2 selectable levels (H: over 1.0 V, L: 0 - 0.5 V), (H: over 4.0 V, L: 0 - 1.5 V)  |                   |                       |
| Pulse input period                    | With filter OFF: 200 $\mu$ s or more (both H and L periods must be at least 100 $\mu$ s)<br>With filter ON: 100 ms or more (both H and L periods must be at least 50 ms)  |                   |                       |
| Slope                                 | Rising or falling edge can be set for each channel  |                   |                       |
| Pulse measurement mode                | Totalized pulses: Integrated (pulse count integration from start), Instantaneous (pulse count value at each sampling, and integrated value is reset each time)<br>Rotation count: Count input pulses during one second  |                   |                       |
| Filter                                | For contact bound resistant (ON/OFF set for each channels)  |                   |                       |
| Measurement parameters                |   |                   |                       |
|                                       | Ranges  | Finest Resolution | Range of Measurements |
| Pulse totalization                    | 1,000 M (pulse) f.s.  | 1 (pulse)         | 0 to 1,000 M (pulse)  |
| Pulse rotations                       | 5,000/n (r/s) f.s.  | 1/n (r/s)         | 0 to 5,000/n (r/s)    |
|                                       | "n" above is the number of sensor output pulses per rotation, 1 to 1,000  |                   |                       |
| Digital input                         | Record logical "1" or "0" at each sampling  |                   |                       |

## Product Specifications

| Analog input section (@23 ±5°C/73 ±9°F, 80% rh or less, after 30 minutes of warm-up and zero-adjustment, with the 50/60 Hz cut-off setting selected) |  |  |                          |          |
|--|--|--|--------------------------|----------|
| Voltage Setting Ranges   | Resolution   | Measurement range  | Accuracy                 |          |
| 10 mV f.s.   | 500 nV   | -10 mV to 10 mV  | ±10 μV                   |          |
| 20 mV f.s.   | 1 μV   | -20 mV to 20 mV  | ±20 μV                   |          |
| 100 mV f.s.  | 5 μV   | -100 mV to 100 mV  | ±100 μV                  |          |
| 200 mV f.s.  | 10 μV  | -200 mV to 200 mV  | ±200 μV                  |          |
| 1 V f.s.   | 50 μV  | -1 V to 1 V  | ±1 mV                    |          |
| 2 V f.s.   | 100 μV   | -2 V to 2 V  | ±2 mV                    |          |
| 10 V f.s.  | 500 μV   | -10 V to 10 V  | ±10 mV                   |          |
| 20 V f.s.  | 1 mV   | -20 V to 20 V  | ±20 mV                   |          |
| 100 V f.s.   | 5 mV   | -100 V to 100 V  | ±100 mV                  |          |
| 1 – 5 V f.s.   | 500 μV   | 1 V to 5 V   | ±10 mV                   |          |
| Temperature Thermocouples (Excluding standard reference contact accuracy)  |  | (Compliance standard)<br>K, J, E, T, N, R, S, B : JIS C1602-1995, IEC 584<br>W : ASTM E-988-96 |                          |          |
| Thermocouple   | Setting Ranges   | Resolution   | Measurement range        | Accuracy |
| K  | 100°C f.s.   | 0.01°C   | -100 to less than 0°C    | ±0.8°C   |
|  |  |  | 0 to 100°C               | ±0.6°C   |
|  | 500°C f.s.   | 0.05°C   | -200 to less than -100°C | ±1.5°C   |
|  |  |  | -100 to less than 0°C    | ±0.8°C   |
|  |  |  | 0 to 500°C               | ±0.6°C   |
|  | 2000°C f.s.  | 0.1°C  | -200 to less than -100°C | ±1.5°C   |
| J  | 100°C f.s.   | 0.01°C   | -100 to less than 0°C    | ±0.8°C   |
|  |  |  | 0 to 100°C               | ±0.6°C   |
|  | 500°C f.s.   | 0.05°C   | -200 to less than -100°C | ±1.0°C   |
|  |  |  | -100 to less than 0°C    | ±0.8°C   |
|  |  |  | 0 to 500°C               | ±0.6°C   |
|  | 2000°C f.s.  | 0.1°C  | -200 to less than -100°C | ±1.0°C   |
| E  | 100°C f.s.   | 0.01°C   | -100 to less than 0°C    | ±0.8°C   |
|  |  |  | 0 to 100°C               | ±0.6°C   |
|  | 500°C f.s.   | 0.05°C   | -200 to less than -100°C | ±1.0°C   |
|  |  |  | -100 to less than 0°C    | ±0.8°C   |
|  |  |  | 0 to 500°C               | ±0.6°C   |
|  | 2000°C f.s.  | 0.1°C  | -200 to less than -100°C | ±1.0°C   |
| T  | 100°C f.s.   | 0.01°C   | -100 to less than 0°C    | ±0.8°C   |
|  |  |  | 0 to 100°C               | ±0.6°C   |
|  | 500°C f.s.   | 0.05°C   | -200 to less than -100°C | ±1.5°C   |
|  |  |  | -100 to less than 0°C    | ±0.8°C   |
|  |  |  | 0 to 400°C               | ±0.6°C   |
|  | 2000°C f.s.  | 0.1°C  | -200 to less than -100°C | ±1.5°C   |
| N  | 100°C f.s.   | 0.01°C   | -100 to less than 0°C    | ±1.2°C   |
|  |  |  | 0 to 100°C               | ±1.0°C   |
|  | 500°C f.s.   | 0.05°C   | -200 to less than -100°C | ±2.2°C   |
|  |  |  | -100 to less than 0°C    | ±1.2°C   |
|  |  |  | 0 to 500°C               | ±1.0°C   |
|  | 2000°C f.s.  | 0.1°C  | -200 to less than -100°C | ±2.2°C   |
|  |  | -100 to less than 0°C  | ±1.2°C                   |          |
|  |  | 0 to 1300°C  | ±1.0°C                   |          |
| Thermocouple   | Setting Ranges   | Resolution   | Measurement range        | Accuracy |
| R  | 100°C f.s.   | 0.01°C   | 0 to 100°C               | ±4.5°C   |
|  | 500°C f.s.   | 0.05°C   | 0 to less than 100°C     | ±4.5°C   |
|  |  |  | 100 to less than 300°C   | ±3.0°C   |
|  |  |  | 300 to 500°C             | ±2.2°C   |
|  | 2000°C f.s.  | 0.1°C  | 0 to less than 100°C     | ±4.5°C   |
|  |  |  | 100 to less than 300°C   | ±3.0°C   |
| S  | 100°C f.s.   | 0.01°C   | 0 to 100°C               | ±4.5°C   |
|  | 500°C f.s.   | 0.05°C   | 0 to less than 100°C     | ±4.5°C   |
|  |  |  | 100 to less than 300°C   | ±3.0°C   |
|  |  |  | 300 to 500°C             | ±2.2°C   |
|  | 2000°C f.s.  | 0.1°C  | 0 to less than 100°C     | ±4.5°C   |
|  |  |  | 100 to less than 300°C   | ±3.0°C   |
| B  | 2000°C f.s.  | 0.1°C  | 400 to less than 600°C   | ±5.5°C   |
|  |  |  | 600 to less than 1000°C  | ±3.8°C   |
|  |  |  | 1000 to 1800°C           | ±2.5°C   |
| W  | 100°C f.s.   | 0.01°C   | 0 to 100°C               | ±1.8°C   |
|  | 500°C f.s.   | 0.05°C   | 0 to 500°C               | ±1.8°C   |
|  | 2000°C f.s.  | 0.1°C  | 0 to 2000°C              | ±1.8°C   |
| <b>Other specifications about thermocouple measurement</b>   |  |  |                          |          |
| Reference junction compensation  | Internal/ External, at INT RJC, total accuracy = add ± 0.5°C |  |                          |          |
| Thermocouple burn-out detection  | ON/ OFF, detect at each sampling (when slower than 20 ms)    |  |                          |          |
| Temperature Platinum resistance temperature sensor   |  | (Compliance standard)<br>Pt 100 : JIS C1604-1997, IEC 751, JPt 100 : JIS C1604-1989            |                          |          |
| Types  | Setting Ranges   | Resolution   | Measurement range        | Accuracy |
| Pt 100   | 100°C f.s.   | 0.01°C   | -100 to 100°C            | ±0.6°C   |
|  | 500°C f.s.   | 0.05°C   | -200 to 500°C            | ±0.8°C   |
|  | 2000°C f.s.  | 0.1°C  | -200 to 800°C            | ±1.0°C   |
| JPt 100  | 100°C f.s.   | 0.01°C   | -100 to 100°C            | ±0.6°C   |
|  | 500°C f.s.   | 0.05°C   | -200 to 500°C            | ±0.8°C   |
|  | 2000°C f.s.  | 0.1°C  | -200 to 500°C            | ±1.0°C   |
| Resistance /testing current 1 mA   | Resolution   | Measurement range  | Accuracy                 |          |
| 10 Ω f.s.  | 0.5 mΩ   | 0 to 10 Ω  | ±10 mΩ                   |          |
| 20 Ω f.s.  | 1 mΩ   | 0 to 20 Ω  | ±20 mΩ                   |          |
| 100 Ω f.s.   | 5 mΩ   | 0 to 100 Ω   | ±100 mΩ                  |          |
| 200 Ω f.s.   | 10 mΩ  | 0 to 200 Ω   | ±200 mΩ                  |          |
| Humidity (use sensor Z2000)  | Resolution   | Measurement range  | Accuracy                 |          |
| 100%rh f.s.  | 0.1%rh   | 5.0 to 95.0%rh   | Refer to table below     |          |

■ Humidity sensor Z2000 accuracy

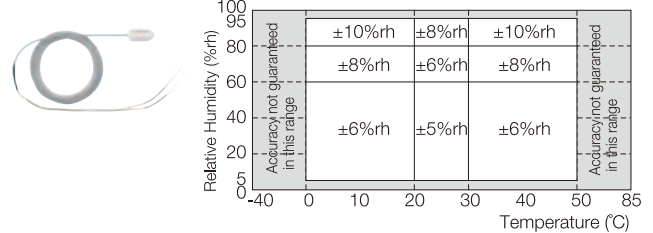

| Filter function (Thermocouple/ Resistance temperature sensor/ Voltage/ Resistance/ Humidity) |  |
|--|--|
| Digital filter   | Select OFF/ 50 Hz/ 60 Hz (In order to remove harmonic components, during analog input the cut-off frequency is automatically set according to the sampling rate) |







## Optional Product Specifications



| VOLTAGE/TEMP UNIT LR8500 (Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year) |   |
|---|---|
| Number of input channels  | 15 channels (input type selectable from voltage, thermocouple, humidity, for each channel), M3 screw terminals (2 terminals per channel)<br><i>Note: Isolated from each channel to chassis</i>  |
| Measurement parameters  | Voltage, Temperature with thermocouples (K, J, E, T, N, R, S, B, W)<br><i>Note: Isolated between channels and from each channel to chassis</i><br>Humidity with the sensor Z2000<br><i>Note: Not isolated between channels nor from each channel to chassis</i> |
| Input conditions  | Input resistance: 1 MΩ (at voltage/ thermocouple measurement)<br>Max. rating: ±100 V DC (max. voltage between input terminals without damage)   |
| Max. rated voltage between isolated input channels  | 250 V DC (max. voltage between input channel terminals)   |
| Max. rated voltage from isolated terminals to ground  | 300 V AC, DC (max. voltage from terminals to chassis ground without damage)   |
| Measurement accuracy  | Refer to MEMORY HILOGGER main unit specifications   |
| Dimensions & Mass   | Approx. 128 mm (5.04 in) W × 52.8 mm (2.08 in) H × 64.5 mm (2.54 in) D, 380 g (13.4 oz)   |



| UNIVERSAL UNIT LR8501 (Accuracy guaranteed for 1 year, Post-adjustment accuracy guaranteed for 1 year) |   |
|--|---|
| Number of input channels   | 15 channels (input type selectable from voltage, thermocouple, Pt 100/ JPt 100, humidity, resistance, for each channel), Push-button type terminals (4 terminals per channel)<br><i>Note: Isolated from each channel to chassis</i>   |
| Measurement parameters   | Voltage, Temperature with thermocouples (K, J, E, T, N, R, S, B, W)<br><i>Note: Isolated between channels and from each channel to chassis</i><br>Platinum resistance temperature sensor (Pt 100, JPt 100, 3-wired/ 4-wired, testing current 1 mA) <i>Note: Not isolated between channels</i><br>Resistance (4-wired, testing current 1 mA) <i>Note: Not isolated between channels</i><br>Humidity with the sensor Z2000<br><i>Note: Not isolated between channels nor from each channel to chassis</i> |
| Input conditions   | Input resistance: 1 MΩ (at voltage/ thermocouple measurement), 2 MΩ (at platinum resistance temperature sensor, or resistance measurement)<br>Max. rating: ±100 V DC (max. voltage between input terminals without damage)  |
| Max. rated voltage between isolated input channels   | 300 V DC (max. voltage between input channel terminals)   |
| Max. rated voltage from isolated terminals to ground   | 300 V AC, DC (max. voltage from terminals to chassis ground without damage)   |
| Measurement accuracy   | Refer to MEMORY HILOGGER main unit specifications   |
| Dimensions & Mass  | Approx. 128 mm (5.04 in) W × 52.8 mm (2.08 in) H × 64.5 mm (2.54 in) D, 300 g (10.6 oz)   |

| Model Line-up  |  |   |
|--|--|---|
| Items  | Specifications   | Model LR8400-20 (built-in the Voltage/temp unit LR8500 ×2, 30 ch)   |
| Analog input   | Built-in 30 channels <i>Note: Isolated from each channel to chassis</i><br>[UNIT-1, UNIT-2] M3 screw terminals × 30 channels (2 terminals per channel)   | <b>Caution: Built-in M3 screw terminal units cannot be removed or replaced</b>                              |
|  | Expandable by adding 30 more channels for a total of 60 input channels (optional input unit, Model LR8500 or LR8501, up to 2 units)  |   |
| Measurement parameters                               | Voltage, Temperature with thermocouples (K, J, E, T, N, R, S, B, W)<br><i>Note: Isolated between channels and from each channel to chassis</i><br>Humidity with the sensor Z2000<br><i>Note: Not isolated between channels nor from each channel to chassis</i>  |                          |
| Input resistance                                     | 1 MΩ (at voltage/ thermocouple measurement)  |   |
| Max. allowable input                                 | ±100 V DC (max. voltage between input terminals without damage)  |                          |
| Max. rated voltage between isolated input channels   | 250 V DC (max. voltage between input channel terminals)  |   |
| Max. rated voltage from isolated terminals to ground | 300 V AC, DC (max. voltage from terminals to chassis ground without damage)  |   |
| Items  | Specifications   | Model LR8401-20 (built-in the Universal unit LR8501 ×2, 30 ch)  |
| Analog input   | Built-in 30 channels <i>Note: Isolated from each channel to chassis</i><br>[UNIT-1, UNIT-2] Push-button type terminals × 30 channels (4 terminals per channel)   | <b>Caution: Built-in push-button terminal units cannot be removed or replaced</b>                           |
|  | Expandable by adding 30 more channels for a total of 60 input channels (optional input unit, Model LR8500 or LR8501, up to 2 units)  |   |
| Measurement parameters                               | Voltage, Temperature with thermocouples (K, J, E, T, N, R, S, B, W)<br><i>Note: Isolated between channels and from each channel to chassis</i><br>Platinum resistance temperature sensor (Pt 100, JPt 100, 3-wired/ 4-wired, testing current 1 mA)<br><i>Note: Not isolated between channels</i><br>Resistance (4-wired, testing current 1 mA) <i>Note: Not isolated between channels</i><br>Humidity with the sensor Z2000<br><i>Note: Not isolated between channels nor from each channel to chassis</i> |                          |
| Input resistance                                     | 1 MΩ (at voltage/ thermocouple measurement)<br>2 MΩ (at resistance temperature sensor, or resistance measurement)  |   |
| Max. allowable input                                 | ±100 V DC (max. voltage between input terminals without damage)  |                          |
| Max. rated voltage between isolated input channels   | 300 V DC (max. voltage between input channel terminals)  |   |
| Max. rated voltage from isolated terminals to ground | 300 V AC, DC (max. voltage from terminals to chassis ground without damage)  |   |
| Items  | Specifications   | Model LR8402-20 (built-in the Universal unit ×1, Voltage/temp unit ×1, 30 ch)                               |
| Analog input   | Built-in 30 channels <i>Note: Isolated from each channel to chassis</i><br>[UNIT-1] Push-button type terminals × 15 channels (4 terminals per channel)<br>[UNIT-2] M3 screw terminals × 15 channels (2 terminals per channel)  | <b>Caution: Built-in push-button terminal unit and M3 screw terminal unit cannot be removed or replaced</b> |
|  | Expandable by adding 30 more channels for a total of 60 input channels (optional input unit, Model LR8500 or LR8501, up to 2 units)  |   |
| Measurement parameters                               | Voltage, Temperature with thermocouples (K, J, E, T, N, R, S, B, W)<br><i>Note: Isolated between channels and from each channel to chassis</i><br>Humidity with the sensor Z2000<br><i>Note: Not isolated between channels nor from each channel to chassis</i><br>[UNIT-1 side only] Platinum resistance temperature sensor (Pt 100, JPt 100, 3-wired/ 4-wired) <i>Note: Not isolated between channels</i><br>Resistance (4-wired) <i>Note: Not isolated between channels</i>                             |                        |
| Input resistance                                     | 1 MΩ (at voltage/ thermocouple measurement)<br>2 MΩ (at platinum resistance temperature sensor, or resistance measurement)   |   |
| Max. allowable input                                 | ±100 V DC (max. voltage between input terminals without damage)  |                        |
| Max. rated voltage between isolated input channels   | 250 V DC at M3 screw terminals, 300 V DC at push-button type terminals (max. voltage between input channel terminals)  |   |
| Max. rated voltage from isolated terminals to ground | 300 V AC, DC (max. voltage from terminals to chassis ground without damage)  |   |

## Software specifications


| Logger Utility SF1000 (bundled application software) |   |
|--|---|
| Supported units                                      | Model 8423, 8430, LR8431, LR8432, LR8400, LR8401, LR8402, and LR8410  |
| Operating environment                                | Windows 10/8/7 (32bit/64bit), Vista (32bit/64bit), XP (with SP2 or later) (32bit)   |
| Real-time data acquisition                           | Measurements on multiple loggers connected by LAN or USB can be controlled to sequentially acquire, display and save waveform data (for recording up to 10 million samples)<br>Number of controllable instruments: up to 5 units<br>(This software is compatible only with the LR8410-20, LR8400-20series, LR8431-20, 8423, and 8430-20)<br>Display: Waveforms (time-axis divided display possible), numerical values (logging), and alarm status can be displayed at the same time<br>Numerical value display: Can be monitored in a separate window<br>Scroll: Waveform scroll while measuring<br>Data saving destination: Real-time data transfer to Excel, or Real-time data acquisition file (LUW format)<br>Event marks: Can be set while measuring |
| Data acquisition settings                            | Data acquisition settings for the logger or logging station<br>Saving: The setting for multiple loggers or logging stations can be saved together in one file (LUS format); Instrument configuration settings can be sent and received  |
| Waveform display                                     | Processed data file: Real-time data acquisition file (LUW format), Record to internal memory data (MEM format)<br>Display format: Simultaneously display waveform and numerical value, (time-axis divided display possible)<br>Maximum number of channels: 675 channels (measurement data) + 60 channels (waveform processing data)<br>Others: Display each channel's waveform on 10 sheets, scroll, record event mark, cursor, screen hard copy, numerical value display   |



|                        |   |
|------------------------|---|
| Data conversion        | Target data: Real-time data acquisition file (LUW format), record to internal memory data (MEM format)<br>Converted sections: All data, designation section<br>Format: CSV format (separate by comma, space, tab), transfer to Excel spreadsheet, arbitrary data thinning   |
| Waveform processing    | Processing items: Four arithmetic operations<br>Number of processing channels: 60 channels  |
| Parameter calculations | Target data: Real-time data acquisition file (LUW format), record to internal memory data (MEM format), data acquired in real time, waveform processing data<br>Calculation items: Average, peak, maximum values, time to maximum values, minimum values, time to minimum values, ON time, OFF time, count the number of ON time and OFF time, standard deviation, integration, area values, totalization |
| Search functions       | Target data: Real-time data acquisition file (LUW format), record to internal memory data (MEM format)<br>Search mode: Event mark, time and date, maximum position, minimum position, maximum pole, minimum pole, alarm position, level, window, amount of change   |
| Print functions        | Supported printer: Printer compatible with the OS<br>Target data: Real-time data acquisition file (LUW format), record to internal memory data (MEM format)<br>Print format: Waveform image, report format, list print (channel settings, event, cursor value)<br>Print area: The entire area, area between cursors A and B<br>Print preview: Supported   |



## Main units

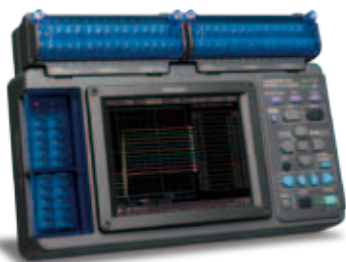

### Model : MEMORY HiLOGGER LR8400

Model No. (Order Code) (Note)

**LR8400-20** (built-in the Voltage/temp unit LR8500 ×2, 30 ch)

*Caution: Built-in units cannot be removed or changed. The Battery pack Z1000 is sold separately.*

Model LR8400 : Built-in units are equivalent to the Voltage/temp unit LR8500 × 2  
Bundled Accessories: Detailed operating manual ×1, Measurement guide ×1, AC ADAPTER 9418-15 ×1, USB cable ×1, CD-R (data collection software "Logger Utility") ×1



### Model : MEMORY HiLOGGER LR8401

Model No. (Order Code) (Note)

**LR8401-20** (built-in the Universal unit LR8501 ×2, 30 ch)

*Caution: Built-in units cannot be removed or changed. The Battery pack Z1000 is sold separately.*

Model LR8401 : Built-in units are equivalent to the Universal unit LR8501 × 2  
Bundled Accessories: Detailed operating manual ×1, Measurement guide ×1, AC ADAPTER 9418-15 ×1, USB cable ×1, CD-R (data collection software "Logger Utility") ×1



### Model : MEMORY HiLOGGER LR8402

Model No. (Order Code) (Note)

**LR8402-20** (built-in the Voltage/temp unit ×1, Universal unit ×1, 30 ch)

*Caution: Built-in units cannot be removed or changed. The Battery pack Z1000 is sold separately.*

Model LR8402 : Built-in units are equivalent to the Voltage/temp unit LR8500 (15 ch) × 1, and the Universal unit LR8501 (15 ch) × 1

Bundled Accessories: Detailed operating manual ×1, Measurement guide ×1, AC ADAPTER 9418-15 ×1, USB cable ×1, CD-R (data collection software "Logger Utility") ×1

## LR8400-20/LR8401-20/LR8402-20 Options in Detail

|   |   |  |
|---|---|--|
| <p><b>Input modules</b></p> <p><b>VOLTAGE/TEMP UNIT LR8500</b><br/>2 terminals M-3 mm screw type, 15 channels, Voltage, Temperature with thermocouple, or Humidity measurement, for the LR8400 series</p> <p><b>UNIVERSAL UNIT LR8501</b><br/>4 terminals push-button type, 15 channels, Voltage, Temperature with thermocouple, Platinum Resistance temperature sensor, Humidity, or Resistance measurement, for the LR8400 series</p> | <p><b>Input options</b></p> <p><b>HUMIDITY SENSOR Z2000</b><br/>3 m (9.84 ft) length</p> <p><b>Thermocouple</b><br/>*For reference only. Please purchase locally.</p>   | <p><b>Storage media</b></p> <p><b>PC Card Precaution</b><br/>Use only PC Cards sold by HIOKI. Compatibility and performance are not guaranteed for PC cards made by other manufacturers. You may be unable to read from or save data to such cards.</p> <p>* Supplied with PC Card adapter</p> <p><b>PC CARD 2G 9830</b><br/>2 GB capacity</p> <p><b>PC CARD 1G 9729</b><br/>1 GB capacity</p> <p><b>PC CARD 512M 9728</b><br/>512 MB capacity</p> |
| <p><b>Power supply</b></p> <p><b>BATTERY PACK Z1000</b><br/>NiMH. Charges while installed in the main unit</p> <p><b>AC ADAPTER 9418-15</b><br/>100 to 240V AC</p> <p>*AC adapter is bundled with the LR8400 series</p>   | <p><b>Carrying cases and stands</b></p> <p><b>CARRYING CASE C1000</b><br/>Includes compartment for options</p> <p><b>FIXED STAND Z5000</b><br/>For wall hanging and slanted bench mounting</p>  | <p><b>For the PC</b></p> <p><b>LOGGER UTILITY SF1000</b><br/>The control of the measurement of loggers, real-time data collection</p> <p><b>LAN CABLE 9642</b><br/>Straight Ethernet cable, supplied with straight to cross conversion adapter, 5 m (16.41 ft) length</p> <p>*LOGGER UTILITY is a bundled software</p>   |
| <p><b>High voltage measurement</b></p> <p><b>DIFFERENTIAL PROBE P9000-01</b><br/>(Waveform mode) For up to 1 kV AC, DC</p> <p><b>DIFFERENTIAL PROBE P9000-02</b><br/>(Waveform / RMS mode selectable) For up to 1 kV AC, DC</p> <p><b>AC ADAPTER Z1008</b><br/>100 to 240 V AC</p> <p>* Maximum input-to-ground rated voltages fall within these products' specifications ranges (and do not affect the connected input units)</p>      | <p><b>Options for Differential Probe</b></p> <p><b>GRABBER CLIP 9243</b><br/>Attaches to the tip of the banana plug cable, 196 mm (7.72 in) length, CAT III 1000 V</p> <p><b>CONVERSION CABLE L1011</b><br/>30 cm (0.98 ft) length, covert BNC to wire</p> <p><b>CONVERSION CABLE L1011-10</b><br/>2.4 m (7.87 ft) length, covert BNC to wire</p> | <p><b>Custom cable</b></p> <p>*For the P9000</p> <p>Inquire with your Hioki distributor.</p> <ol style="list-style-type: none"> <li>(1) Bus powered USB cable</li> <li>(2) USB(A)- Micro B cable</li> <li>(3) 3-prong cable</li> </ol>   |

Note: Company names and Product names appearing in this catalog are trademarks or registered trademarks of various companies.

# HIOKI

HIOKI E. E. CORPORATION

#### HEADQUARTERS

81 Koizumi, Ueda, Nagano, 386-1192, Japan  
TEL +81-268-28-0562 FAX +81-268-28-0568  
http://www.hioki.com / E-mail: os-com@hioki.co.jp

#### HIOKI USA CORPORATION

TEL +1-609-409-9109 FAX +1-609-409-9108  
http://www.hiokiusa.com / E-mail: hioki@hiokiusa.com

HIOKI (Shanghai) SALES & TRADING CO., LTD.  
TEL +86-21-63910090 FAX +86-21-63910360  
http://www.hioki.cn / E-mail: info@hioki.com.cn

DISTRIBUTED BY

HIOKI SINGAPORE PTE. LTD.  
TEL +65-6634-7677 FAX +65-6634-7477  
E-mail: info-sg@hioki.com.sg

HIOKI KOREA CO., LTD.  
TEL +82-2-2183-8847 FAX +82-2-2183-3360  
E-mail: info-kr@hioki.co.jp